

1    **“Screening of Suspected HIV-AIDS Patients: A Comparative Study Evaluating HIV-ICT**  
2    **Device and ELISA”**

3

4

**Abstract**

5    Objectives:

6    To evaluate the sensitivity and specificity of Immunochromatographic device in comparison with  
7    Enzyme Linked Immuno-Sorbent Assay.

8

9    Material and Methods:

10        It was a descriptive comparative study certified by Ethical Review Board of Allama Iqbal  
11    Medical College Lahore. Study was conducted at the Department of Pathology, Allama Iqbal  
12    Medical College Lahore. A total of 106 study subjects were included by using convenient  
13    sampling method within the duration of 4 months. Samples were processed in ELISA section,  
14    Department of Pathology, Allama Iqbal Medical College. Data was entered and analysed by  
15    using SPSS 22.0. A p-value of  $\leq 0.05$  was considered as statistically significant.

16

17    Results:

18    Out of 106 patients 28 samples had been reported as positive with HIV–ELISA whereas, HIV  
19    ICT devices reported 20 cases as positive. On the other hand 78 samples stood negative with  
20    HIV-ELISA and 77 samples remained negative with HIV-ICT device. For HIV ICT device, the  
21    calculated sensitivity was 71.4% and the Specificity was 98.7%. The Positive Predictive Value  
22    (PPV) was 95.2% whereas the Negative Predictive Value (NPV) was 90.6%.

23    Conclusion:

24 The ICT device is a rapid, reliable and valid device with shortest turn-around time and can be  
25 used in emergency settings. Although, the device showed high sensitivity and specificity, but it  
26 cannot be taken as an ultimate diagnostic tool for HIV screening. Final diagnosis should be based  
27 on anti HIV 1/2 ELISA, Western Blot and PCR findings.

28 Key words:

29 Human Immunodeficiency Virus (HIV); Acquired Immunodeficiency Syndrome (AIDS);  
30 Injection Drug Users (IDU); Immunochromatographic Device (ICT); Enzyme Linked  
31 Immunosorbent Assay (ELISA).

### 32 **Introduction**

33 **AIDS** is a retroviral disease caused by Human Immunodeficiency Virus (HIV)  
34 characterized by depletion of CD4+ T-Lymphocytes, which later leads to immunosuppressant,  
35 opportunistic infections, secondary neoplasms and neurologic manifestations [1]. As the  
36 epidemiologic pattern of the disease unfolded, it became clear that an infectious agent  
37 transmissible by sexual (homosexual and heterosexual) contact and blood or blood products was  
38 the most likely etiologic cause of the epidemic [2].

39 In 1983, HIV was isolated from a patient with lymphadenopathy and by 1984 it was  
40 demonstrated clearly to be the causative agent of AIDS [3]. Although AIDS was first described  
41 in United States, it has now been reported in virtually every country in the world. Worldwide,  
42 more than 22 million people have died of AIDS since the epidemic was recognized in 1981.  
43 About 42 million people are living with the disease, and there are estimated 5 million infections  
44 each year. Worldwide 95% of HIV infections are in developing countries, with Africa alone  
45 carrying more than 50% of the HIV burden. AIDS still represents the fifth most common cause  
46 of death in adults between the age of 25 and 44 [1].

47           Prevalence of HIV reached 31% amongst the Injection Drug Users (IDUs) in 2007 in  
48 Karachi, Pakistan making them the most vulnerable group. Males migrating from rural to urban  
49 areas for earning usually get involved in unsafe sexual practices being helped by the emergence  
50 of "red light areas" in the metropolitan cities. Professional blood donors and inadequate blood  
51 screening techniques worsen the scenario [4].

52 Rapid diagnostic tests (RDTs) are diagnostic assays designed for use at the point-of-care (POC)  
53 testing and can be adapted for use in low-resource settings. There are over 60 types of rapid HIV  
54 tests being used around the world [5]. A Rapid Diagnostic Test is low-cost, simple to operate and  
55 read, sensitive, specific, stable at high temperatures, and works in a short period of time [2].  
56 Rapid HIV tests also referred to as rapid/simple (r/s) test devices these tests are based on one of  
57 four immunodiagnostic principles: particle agglutination, immunodot (dipstick),  
58 immunofiltration and immune chromatography [6]. Immunochromatographic device tests are  
59 better than other rapid assays by making HIV diagnostic test a one-step assay [7].

60           Iweala, (2004) reviewed different diagnostic tools for the detection of HIV and stated that  
61 the HIV diagnostic tests that detect host antibody specific to the virus include the enzyme  
62 immunoassay (EIA, also commonly referred to as the enzyme-linked immunosorbent assay),  
63 Western blot (or immunoblot), the immunofluorescence assay (IFA), rapid tests, salivary tests,  
64 urine tests and the detuned assay. Predictive value of the EIA and of HIV screening tests in  
65 general, or the likelihood that the assay will accurately determine a person's true infection status,  
66 depends on the prevalence of HIV infection in the population. In general, the higher the  
67 prevalence of HIV infection in the population, the higher the positive predictive value of the  
68 assay. [7]

69 Butto, (2010) studied different diagnostic tools for HIV and stated that Rapid tests can  
70 present some problems of sensitivity [8]. Kwenti, (2011) conducted a study to determine the  
71 validity of the results obtained by immunochromatographic rapid strip test to diagnose hepatitis  
72 C virus infection in HIV-positive patients and compared it with the results obtained by more  
73 sensitive and specific methods like ELISA and PCR. Evaluation of the rate of false positives  
74 with the rapid strip test using ELISA as the gold standard gave a rate of 6.3% [9].

75 Deguchi, (2012) conducted a study to evaluate the clinical performance of a new assay  
76 against immunochromatographic assay (ICA) for HIV Ab detection, ELISA for Ag/Ab  
77 combination assay and chemiluminescent enzyme immunoassay (CLEIA) for Ab detection and  
78 were evaluated with the immunochromatographic assay for Ag/Ab detection. The study found  
79 that HIV Ag/Ab ICA showed 100% clinical specificity and was better than 99.8% of the existing  
80 ICA. The CLEIA and ELISA showed 100% and 99.8% specificity, respectively [10].

81 Therefore, the present study has been designed to estimate the prevalence of HIV in  
82 patients presenting in 04 months of duration at Jinnah Hospital Lahore/Allama Iqbal Medical  
83 College and to detect the sensitivity and specificity of HIV ICT device in comparison with HIV-  
84 ELISA.

85

86

### **Material and Methods**

87 It was a descriptive comparative study certified by Ethical Review Board of Allama Iqbal  
88 Medical College Lahore. Study was conducted at the department of pathology, Allama Iqbal  
89 Medical College Lahore. Blood samples from a total of 106 study subjects were collected by  
90 using convenient sampling method within the duration of 04 months. Suspected cases of HIV  
91 infection presenting in Department of Pathology, without any discrimination of age or gender

92 were included in this study. Three ml of blood sample from these patients was drawn according  
93 to the WHO protocol. Serum was separated for HIV screening by ELISA and ICT device.  
94 Samples were processed in tertiary care AIDS referral centre and ELISA section, Department of  
95 Pathology, Allama Iqbal Medical College Lahore. ICT device and ELISA kit used, both were  
96 standardized and commercial.

97         ICT device (Alere Global, USA) determines HIV-1/2 is an immunochromatographic test  
98 for the qualitative detection of antibodies to HIV-1 and HIV-2. Sample was added to the sample  
99 pad. As the sample migrated through the conjugate pad, it constituted and got mixed with the  
100 selenium colloid-antigen conjugate. This mixture continued to migrate through the solid phase to  
101 the immobilized recombinant antigens and synthetic peptides at the patient window site.

102         In HIV detection ELISA kit (BioTech Services, Pakistan), a specific antigen was attached  
103 to solid phase by passive adsorption or with antigen specific antibody. Test serum containing  
104 specific antibody was added. Enzyme labeled antiglobulin specific for the test serum was added.  
105 Chromogenic enzyme substrate was then added. The color developed was proportional to the  
106 amount of antibody present in the test serum.

107

108

109

## Results

110         This observational study was undertaken for a period of four months at the Department of  
111 Pathology, Allama Iqbal Medical College, Lahore. Blood samples from a total of 106 patients,  
112 fulfilling the study criteria had been included in the study. The samples were collected from out  
113 patients department, Jinnah Hospital Lahore and patients presented in the Department of  
114 Pathology, Allama Iqbal Medical College and also from Laboratory staff members who were

115 highly suspected for HIV infection specifically the staff dealing with the patients from Punjab  
116 AIDS Control Program (PACP) working in the Flowcytometry section.

117 Fortunately, we have found those highly suspected staff members negative with HIV.  
118 However, samples from Jinnah Hospital were mostly reported Positive and the reason sorted  
119 behind was that these samples were taken from prisoners and they were mostly intravenous drug  
120 users (IDUs) and were involved in extra marital contacts.

121 The mean age of study population was  $34.63 \pm 9.79$  years, ranging between 19 to 60 years  
122 (Median 32.0 and Mode 42.0). Out of 106 samples 83 were males and 23 were females i.e.  
123 78.30% and 21.70% respectively.

124 Out of 106 patients 28 samples had been reported as Positive with HIV-ELISA whereas, HIV  
125 ICT Devices reported 21 cases as Positive. On the other hand 78 samples stood Negative with  
126 HIV-ELISA and 85 samples remained Negative with HIV-ICT Device (Table 1).

127 All the above mentioned statistical data after the application of appropriate statistical tools has  
128 eventually aided us with the calculation of sensitivity and specificity of HIV-ICT Device against  
129 the HIV-ELISA assay. For HIV-ICT device, the calculated sensitivity is 71.4% and the  
130 Specificity is 98.7%. The Positive Predictive Value (PPV) is: 95.2% whereas, the Negative  
131 Predictive Value( NPV) is: 90.6% (Table 1)

132 In a ROC Curve the true positive rate (sensitivity) is plotted in function of the false positive rate  
133 (specificity) for different cut off points of a parameter. Each point on the ROC curve represents a  
134 sensitivity / specificity pair corresponding to a particular decision threshold (Figure 1).

### 135 **Discussion**

136 The main purpose of the present study was the screening of suspected HIV/AIDS patients  
137 and the evaluation of the performance of HIV-ICT device by comparing it with ELISA. After

138 the application of appropriate statistical techniques, results showed the sensitivity and specificity  
139 of HIV-ICT device against the HIV-ELISA assay. The calculated sensitivity was 71.4% and the  
140 Specificity was 98.7%.

141 Cordes and Ryan (1995) compared Enzyme-linked Immunosorbent assay (ELISA) and  
142 Western blot assay which are commonly used laboratory tests for HIV infection. Results found  
143 that both detect antibodies to HIV but ELISA tests have greater than 98% sensitivity and  
144 specificity for HIV-ELISA results are based on detection of antigen-antibody complexes by  
145 using antibodies labeled with an enzyme that produces a color change in the presence of a  
146 specific substrate. Enzyme Linked Immunosorbent assay was also taken as gold standard in the  
147 present study [11].

148 Hua (2006) studied the sensitivity, specificity and the accuracy of the dot  
149 immunochromatography assay (DICA) for HBsAg, Anti-HCV and Anti-HIV methods. The  
150 plasma specimen of 502 patients were tested for HBs Ag, Anti-HCV and Anti-HIV by DICA and  
151 ELISA. The sensitivity and specificity of the two approaches were compared. The study found  
152 that the sensitivity and specificity of DICA are both slightly lower than those of ELISA. Results  
153 showed that as compared with ELISA, 2 false negative and 5 false positive were found in 502  
154 specimens in HBsAg test by DICA. The sensitivity was 96.4%, while the specificity was 98.9%,  
155 and the accuracy was 98.6%. Nine false positive were found in 502 specimens in Anti-HCV test  
156 by DICA, whose sensitivity was 100%, and the specificity was 98.2%, the accuracy was 98.2%.  
157 false positive and no false negative were found in 502 specimens in Anti-HIV test by DICA, the  
158 specificity was 99.6% and the accuracy was 99.6%. False positive and false negative were found  
159 in HBsAg test. The sensitivity of Anti-HCV and Anti-HIV tested by DICA accorded with ELISA  
160 But the specificity of Anti-HCV and Anti-HIV tested by DICA is slightly lower than those by

161 ELISA. The study suggested that final report should be based on ELISA. The present study also  
162 proved that the sensitivity and specificity of the ICT device is less than ELISA [12].

163 Kwenti (2011) conducted a study to determine the validity of the results obtained by  
164 immunochromatographic rapid strip test to diagnose hepatitis C virus infection in HIV-positive  
165 patients and compared it with the results obtained by more sensitive and specific methods like  
166 ELISA and PCR. Among 350 HIV-positive patients, 25 (7.1%) patients were found to be  
167 positive with the rapid strip test of which 3 (12%) were positive with ELISA and all 3 (100%)  
168 positive with the ELISA were also positive with PCR. Evaluation of the rate of false positives  
169 with the rapid strip test using ELISA as the gold standard gave a rate of 6.3%. Meanwhile in the  
170 control group, after screening with the rapid strip test, 39 (11.1%) were positive of whom 6  
171 (15.4%) were positive with the ELISA and 3 (50%) of the 6 positive with the ELISA were also  
172 positive with the PCR. Evaluation of the rate of false positives with the rapid strip test in the  
173 control group using ELISA as the gold standard gave the rate of 9.6% [9].

174 ICT devices are highly useful in emergency settings and point of care (POC) testing.  
175 False positive results with this immunochromatographic rapid strip test for the diagnosis of  
176 hepatitis C virus, HBs Ag and HIV infection are frequent. Therefore, it reinforces the need for a  
177 confirmatory test prior to treatment in hospital settings. It has already been documented that a  
178 positive result for above mentioned conditions got with an immuno-chromatographic rapid strip  
179 test does not warrants that treatment should begin due to possibility of false positive or false  
180 negative results. Therefore the presence of the disease should be investigated further using a  
181 more sensitive and specific assay prior to treatment. Although PCR and western blotting (WB)  
182 assays are very expensive to be incorporated into hospital settings, an ELISA which is less  
183 expensive and more affordable can be implemented to give more valid results. Moreover, a



184 negative result does not exclude the presence of the infection. If symptoms persist, then the  
185 infection should be investigated further with a PCR and WB assays. It is important that diagnosis  
186 should be done together with the patient medical history. The present study also proved ELISA  
187 to be more specific and sensitive than ICT devices.

## 188 **Conclusion**

189 The ICT device is a rapid, reliable and valid device with shortest turnaround time and can  
190 be used in emergency settings and point of care (POC) testing. The device showed high  
191 sensitivity and specificity, but it cannot be taken as an ultimate diagnostic tool for HIV  
192 screening. Final diagnosis should be based on anti HIV 1/2 ELISA, Western Blot and PCR  
193 findings with the correlation of clinical picture of the suspect.

## 194 **References**

- 195 1. Kumar V, Abbas AK, Fausto RN. Robbins Basic Pathology. 8<sup>th</sup>ed. (2007). New Dehli,  
196 Elsevier.
- 197 2. Sirisak N. Diagnostic value Immunochromatographic Test over clinical predictors for  
198 Tuberculosis in HIV patients. Dove Press Journal 2011; 3:237-244.
- 199 3. Fauci AS, Lane HC. Human immunodeficiency virus disease: AIDS and related disorders.  
200 In: Kasper DL, Fauci AS, Longo DL, Braunwald E, Hauser SL, Jameson JL, eds. Harrison's  
201 Principles of Internal Medicine, 17th ed. USA: The McGraw-Hill companies, Inc. 2008;  
202 1137-203.
- 203 4. Rai MA, Warraich HJ, Ali SH, Nerurkar VR. HIV/AIDS in Pakistan: the battle begins.  
204 Retrovirology 2007; 4: 22.
- 205 5. Paul SM, Grimes-Dennis J, Burr CK, Diferdinando GT. Rapid diagnostic testing for HIV:  
206 clinical implications. New Jersey Medicine 2003; 100 (9):11–14.

- 207 6. Ekwueme DU, Pinkerton SD, Holtgrave D, Branson BM. Cost comparison of three HIV  
208 counseling and testing technologies. *American Journal of Preventive Medicine* 2003; 25:112-  
209 121.
- 210 7. Iweala IO. HIV diagnostic tests: an overview. *Contraception* 2004; 70: 141–147
- 211 8. Butto S, Suligoi B, Belasio FE, Raimondo M. Laboratory diagnostics for HIV infection.  
212 *Annali dell'Istituto Superiore di Sanità* 2010; 46 (1) : 24-33.
- 213 9. Kwentí ET, Njouom R, Njunda AL, Lucien H, Kamga F. Comparison of an  
214 Immunochromatographic Rapid Strip Test, ELISA and PCR in the Diagnosis of Hepatitis C  
215 in HIV Patients in Hospital Settings in Cameroon. *Clinical Medicine and Diagnostics* 2011;  
216 1(1): 21-27.
- 217 10. Deguchi M, Yoshioka N, Kagita M, Kita M, Asari S, Honda T, Kobayashi E. Evaluation  
218 of human immunodeficiency virus-1/2 antigen/antibody immunochromatographic assay.  
219 *Clinical Laboratory* 2011; 58: 11-12.
- 220
- 221 11. Cordes RJ, Ryan ME. Pitfalls in HIV testing. Application and limitations of current tests.  
222 *Postgraduate Medicine* 1995; 98 (5):177-80.
- 223 12. Hu DJ, Dondero TJ, Rayfield MA, George JR, Schochetman G, Jaffe HW, Luo CC,  
224 Kalish ML, Weniger BG, Pau CP. The emerging genetic diversity of HIV. The importance of  
225 global surveillance for diagnostics, research, and prevention. *Journal of American Medical*  
226 *Association* 1996; 275(3):210–216.

227

228 **Table 1:** Comparison of ICT Device with ELISA (n=106)


<b>ELISA</b>	
Positive Cases	28 (26.4%)
Negative Cases	78 (73.6%)
<b>ICT</b>	
Positive Cases	21 (19.8%)
Negative Cases	85 (80.2%)
<b>Sensitivity</b>	71.4%
<b>Specificity</b>	98.7%
<b>PPV*</b>	95.2%
<b>NPV**</b>	90.6%

\*Positive Predictive Value: PPV

\*\*Negative Predictive Value: NPV

229 **Figure 1:** Receiver Operating Characteristics (ROC) Curve (n=106)

230

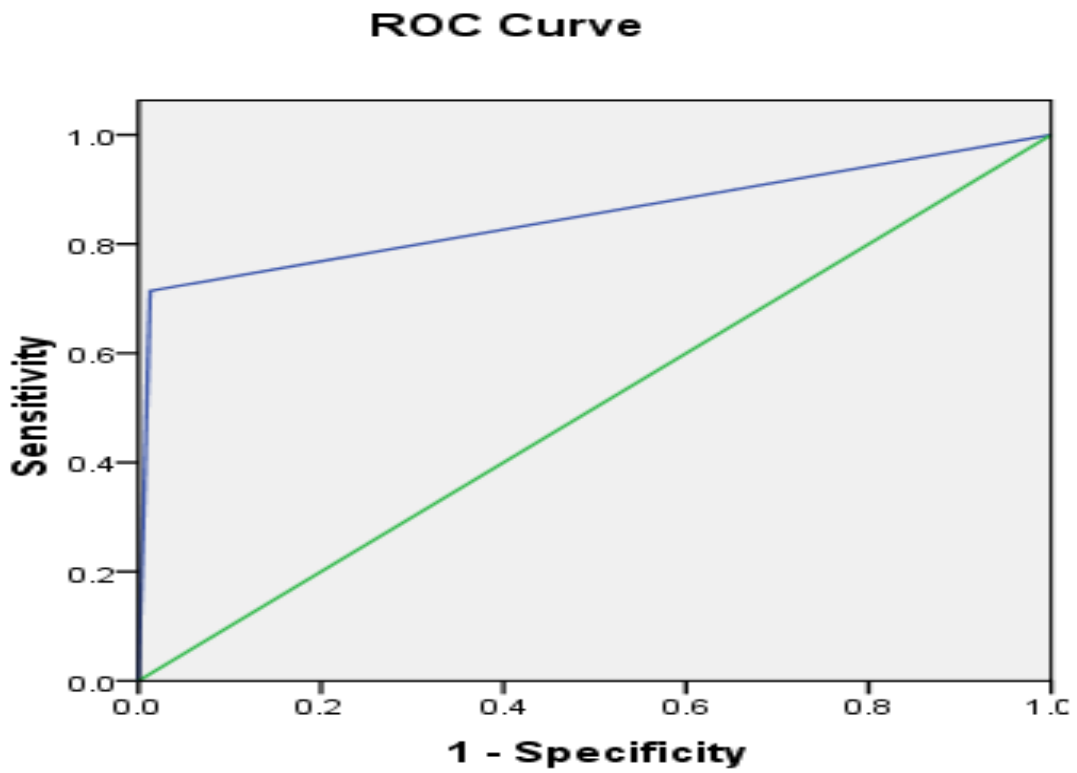

Diagonal segments are produced by ties.

231

232

233

234